



Certificate of Analysis

Name	BioVanta BPC+TB	specs	20mg/3ml (BP) 20mg/3ml (TB)
Lot No.	C-BB40-3.0-20260709	Manufacture Date	2026.07.09
Storage	Store in a dark place and in a sealed container at 2-8℃. Do not freeze.		
Test Items	Acceptance Criteria	Test Results	
【Description】			
Appearance	Colorless to light yellow solution	Conforms	
【Identification】			
HPLC Identification	The retention time of the major peak of the Sample solution corresponds to that of the Standard solution, as obtained in the Assay.	Conforms	
【Test】			
Purity	NLT 95.0% (BP)		99.2%
	NLT 95.0% (TB)		99.5%
Related Substances	BP	Individual impurity NMT2.0%	0.61%
		Total impurities NMT5.0%	0.81%
	TB	Individual impurity NMT2.0%	0.16%
		Total impurities NMT5.0%	0.48%
pH	6.5~7.5		7.0
Phenol Content	4.5mg/mL~5.5mg/mL		5.0mg/mL
Sterility Tests	Meet Requirements		Conforms
Bacterial endotoxins	NMT 20 EU/mg		Less than 20 EU/mg
【Assay】			
Content	≥6.3mg/ml (BP)		7.6mg/ml
	≥6.3mg/ml (TB)		7.4mg/ml
Conclusion: The test results comply with the in-house specification.			

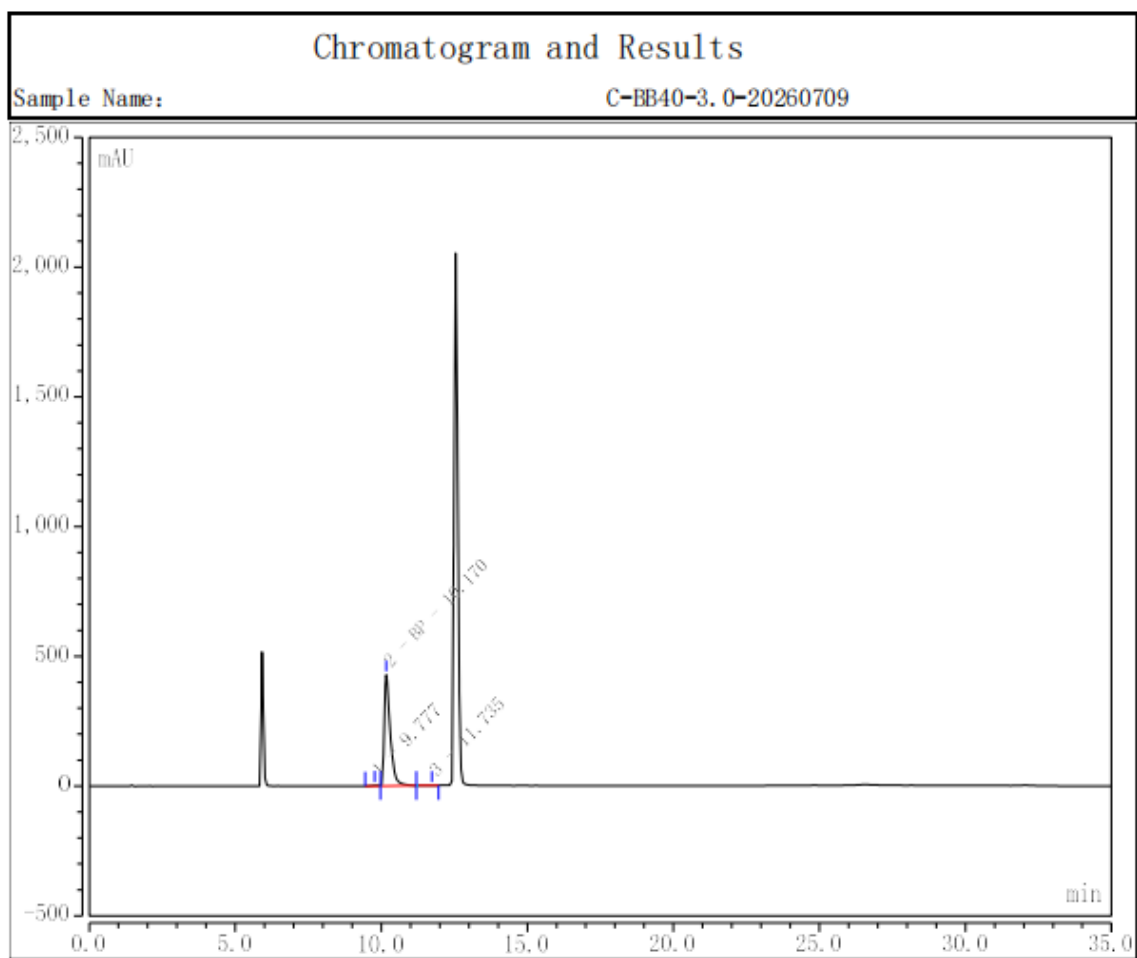

Serial Number	Retention time	Peak name	Peak rel area
	min		%
1	9.78		0.61
2	10.17	BP	99.19
3	11.74		0.20
SUM:			100.00

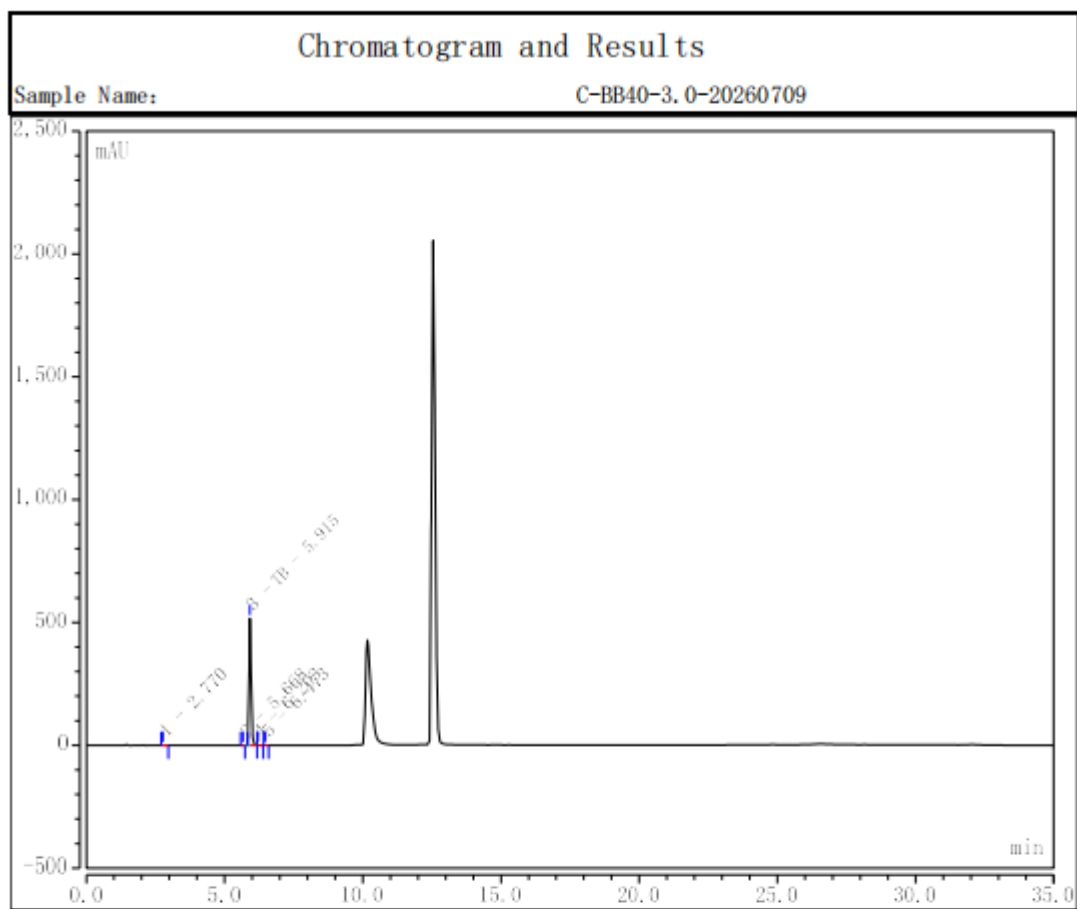

Serial Number	Retention time	Peak name	Peak rel area
	min		%
1	2.77		0.12
2	5.67		0.06
3	5.92	TB	99.52
4	6.20		0.16
5	6.47		0.14
SUM:			100.00