


Certificate of Analysis


Name	BioVanta GLOW	specs	25mg/3ml (GH) 5mg/3ml (TB) 5mg/3ml (BP)
Lot No.	C-GL35-3.0-20260314	Manufacture Date	2026.03.14
Storage	Store in a dark place and in a sealed container at 2-8℃. Do not freeze.		
Test Items	Acceptance Criteria	Test Results	
【Description】			
Appearance	blue solution	Conforms	
【Identification】			
HPLC Identification	The retention time of the major peak of the Sample solution corresponds to that of the Standard solution, as obtained in the Assay.	Conforms	
【Test】			
pH	6.5~7.5	7.0	
Phenol Content	4.5mg/mL~5.5mg/mL	5.0mg/mL	
Sterility Tests	Meet Requirements	Conforms	
Bacterial endotoxins	NMT 20 EU/mg	Less than 20 EU/mg	
【Assay】			
Content	≥7.9mg/ml (GH)	8.8mg/ml	
	≥1.6mg/ml (TB)	1.8mg/ml	
	≥1.6mg/ml (BP)	1.8mg/ml	
Conclusion: The test results comply with the in-house specification.			

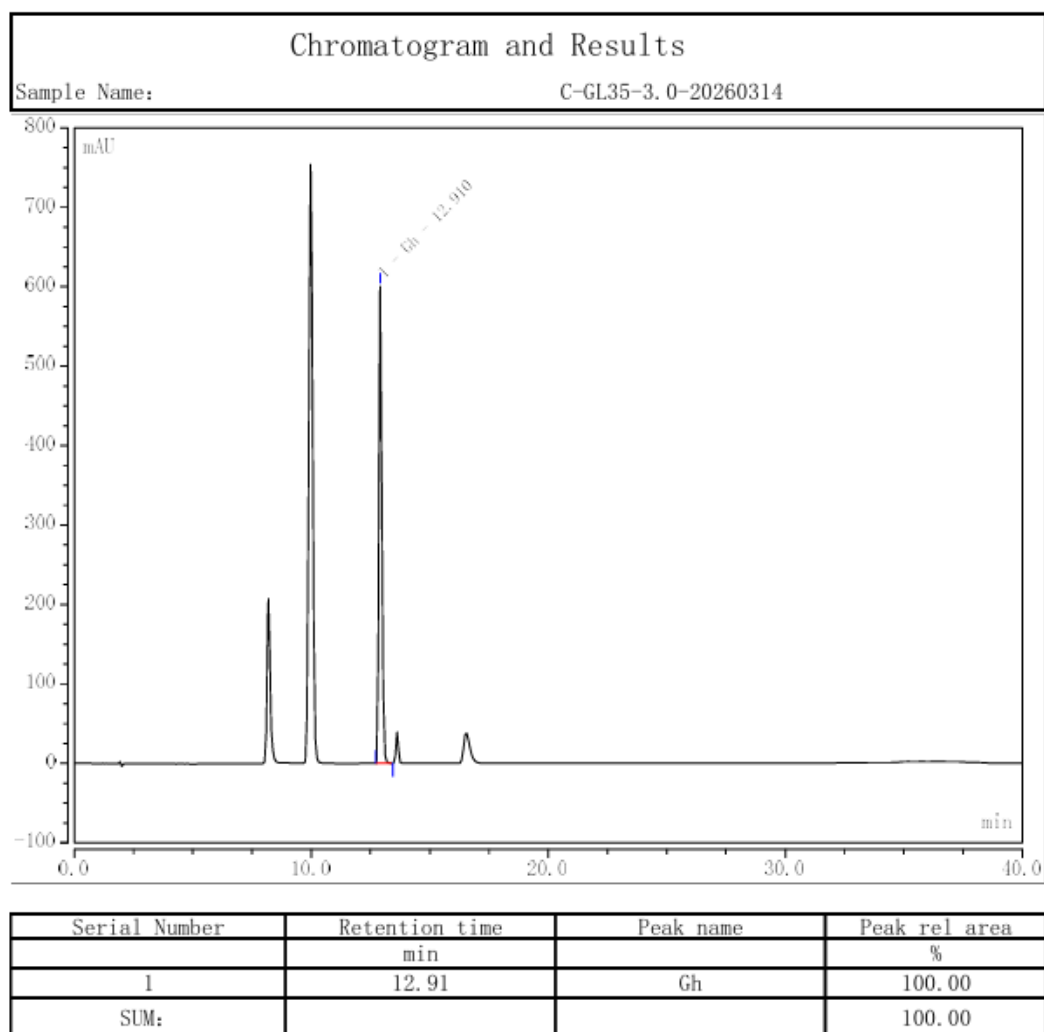

Chromatogram and Results

Sample Name:

C-GL35-3.0-20260314

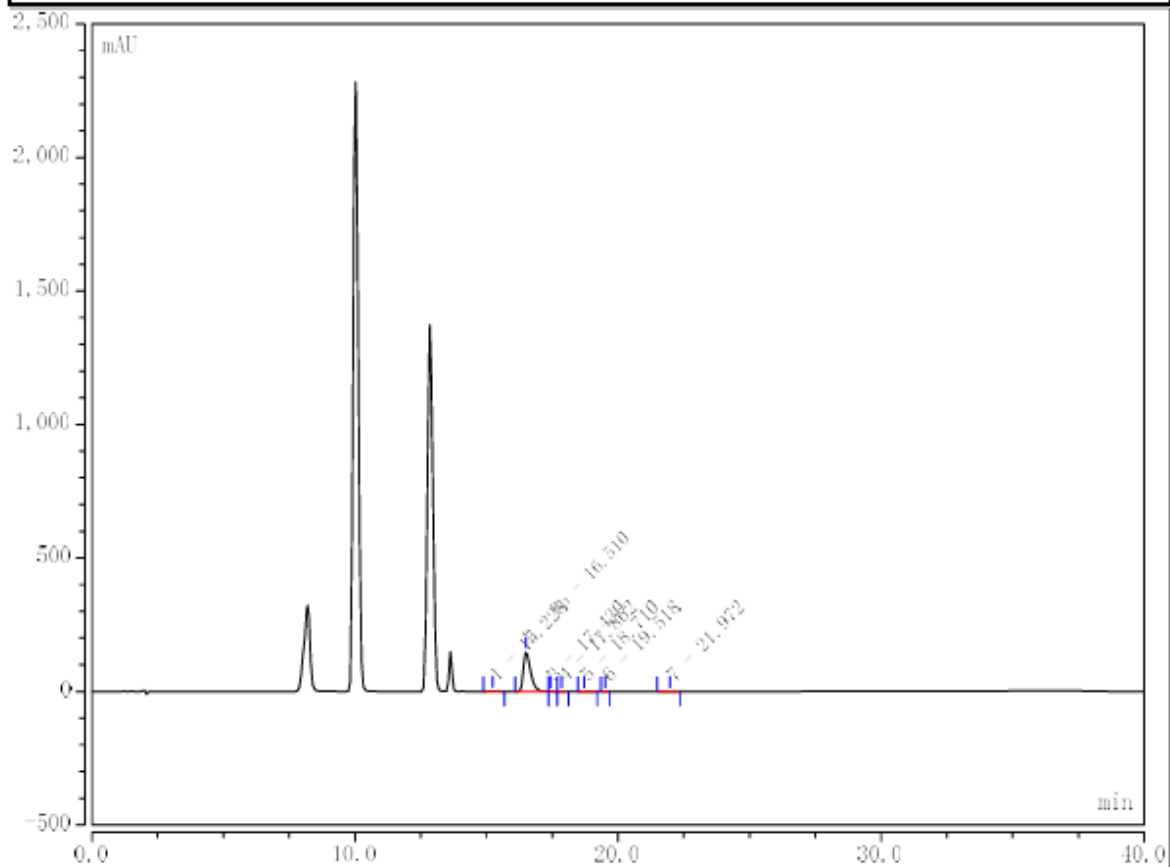


Serial Number	Retention time	Peak name	Peak rel area
	min		%
1	15.23		0.76
2	16.51	Bp	98.89
3	17.43		0.11
4	17.86		0.04
5	18.71		0.07
6	19.52		0.06
7	21.97		0.07
SUM:			100.00

Chromatogram and Results

Sample Name:

C-GL35-3.0-20260314

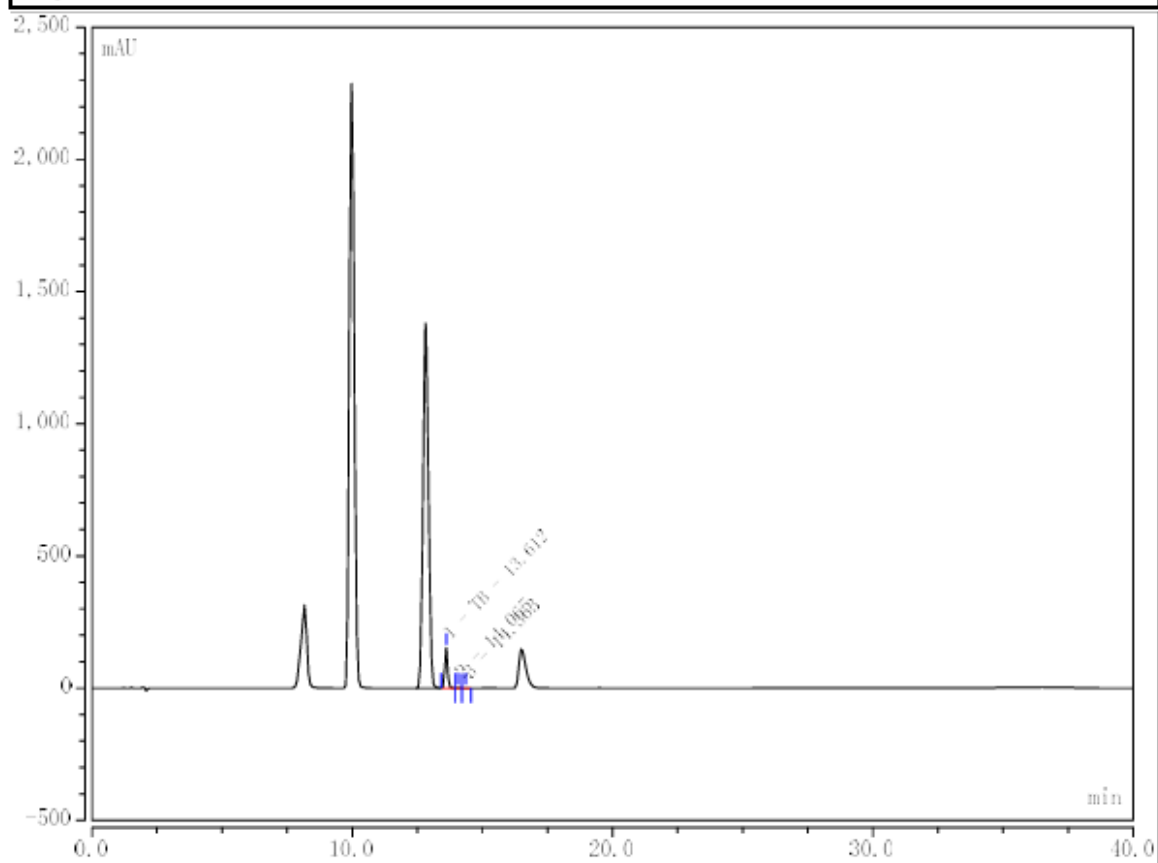

Serial Number	Retention time	Peak name	Peak rel area
	min		%
1	13.61	TB	99.46
2	14.07		0.43
3	14.36		0.11
SUM:			100.00